

Patient's Name:

N°File :

Applicator :

N°apparatus :

Society/Establishment:

Order Date :

Test :

Delivery:

AGE :

WEIGHT :

HEIGHT :

M F

Reserve for sitting :

Abduction Plot Built



The tilt of angle:

Back leg

integrated head rests

(All measurements are the basis of the original seat-braces)

	Width	Depth	Height
Headrest			
Under axis			
Xiphoid			
Height			
Trochanter			

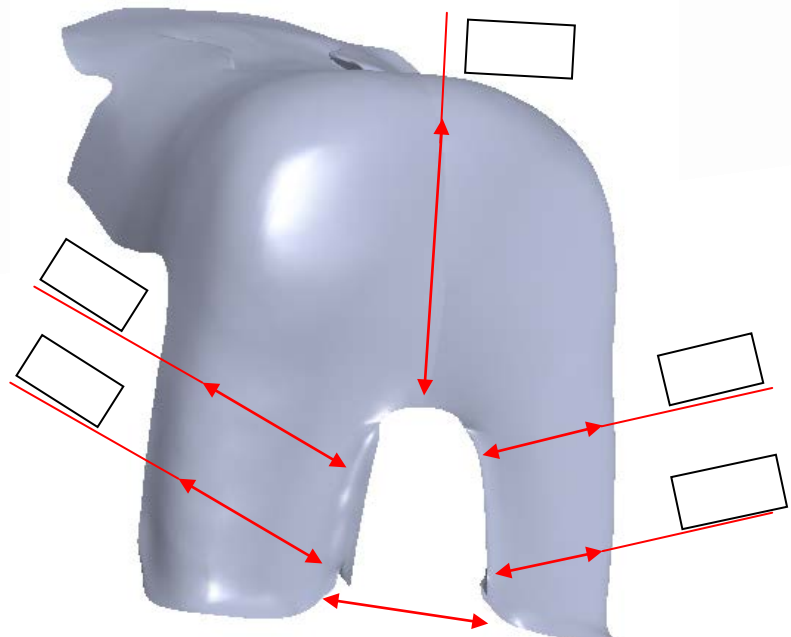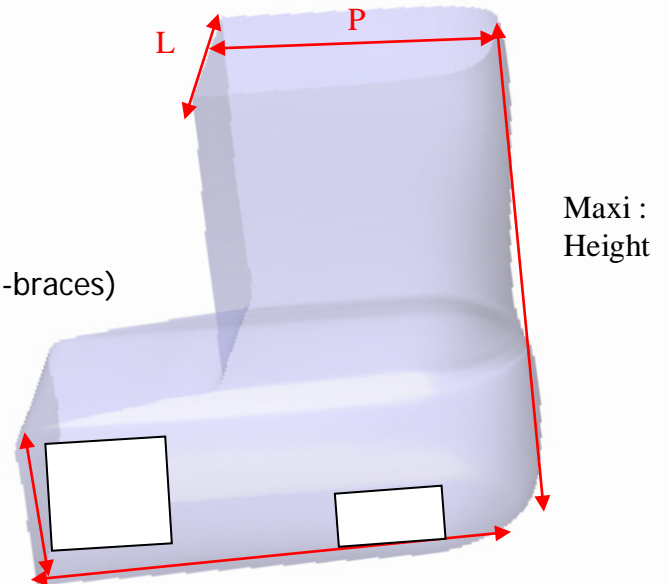

ABDUCTION :

Other information: